

1 **Title:** Skill assessment in upper limb myoelectric prosthesis users: Validation of a clinically feasible
2 method for characterising upper limb temporal and amplitude variability during the performance of
3 functional tasks.

4
5 **Authors:** Sibylle B Thies¹, Laurence PJ Kenney¹, Mohammad Sobuh^{1,2}, Adam Galpin¹, Peter Kyberd³,
6 Rebecca Stine^{4,5}, Matthew J Major^{4,5}

7
8 **Affiliations:**

9 ¹School of Health Sciences, University of Salford, UK; ²Department of Orthotics and Prosthetics, The
10 University of Jordan, Jordan; ³Engineering Science, University of Greenwich, UK; ⁴Northwestern
11 University Prosthetics-Orthotics Center, Northwestern University Feinberg School of Medicine, Chicago,
12 IL, USA; ⁵Jesse Brown VA Medical Center, Chicago, IL, USA

13
14 **Contact information for corresponding author:**

15 **Sibylle Thies**

16 School of Health Sciences
17 Brian Blatchford Building Room PO28
18 The University of Salford
19 Salford, Greater Manchester, M6 6PU, UK

20 **Email:** s.thies@salford.ac.uk

21
22 **Abstract word count:** 200

23 **Manuscript word count:** 3364 (without references), 2 Tables, 5 Figures.

24

25 **ABSTRACT (200 words)**

26 Upper limb myoelectric prostheses remain challenging to use and are often abandoned. A proficient
27 user must be able to plan/execute arm movements while activating the residual muscle(s), accounting
28 for delays and unpredictability in prosthesis response. There is no validated, low cost measure of skill in
29 performing such actions. Trial-trial variability of joint angle trajectories measured during functional task
30 performance, linearly normalised by time, shows promise. However, linear normalisation of time
31 introduces errors, and expensive camera systems are required for joint angle measurements.

32 This study investigated whether trial-trial variability, assessed using dynamic time warping (DTW)
33 of limb segment acceleration measured during functional task performance, is a valid measure of user
34 skill. Temporal and amplitude variability of forearm accelerations were determined in 1) seven
35 myoelectric prosthesis users and six anatomically-intact controls and 2) seven anatomically-intact
36 subjects learning to use a prosthesis simulator over repeated sessions.

37 1: temporal variability showed clear group differences ($p < 0.05$). 2: temporal variability
38 considerably increased on first use of a prosthesis simulator, then declined with training (both $p < 0.05$).
39 Amplitude variability showed less obvious differences. Analysing forearm accelerations using DTW
40 appears to be a valid low-cost method for quantifying movement quality of upper limb prosthesis use
41 during goal-oriented task performance.

42

43 **Keywords**

44 Myoelectric prostheses, dynamic time warping, accelerations, variability, upper limb.

45

46 1. INTRODUCTION

47 As a result of concerted efforts over recent decades, there have been significant advances in myoelectric
48 prostheses design. The motors used have become smaller and more powerful, cosmetic covers have
49 become more life-like, and, of most note, multi-functional hands, such as the i-Limb (Touch Bionics,
50 Livingston, UK) and Be-Bionic (Steeper, Leeds, UK) have been developed. Yet, prosthesis users are still
51 greatly limited by the available control modalities and lack of sensory feedback from the prosthesis [1].
52 Hence it is not surprising that such devices remain challenging to use and are often poorly utilized, or
53 rejected [2, 3]. As more expensive multi-function myoelectric prostheses have become available, such as
54 the i-limb full hand and i-limb digits (Touchbionics Inc., Livingston UK), there is an urgent need for well-
55 validated and robust quantitative measures that allow for informed selection of a particular technology
56 (to achieve a better match between user and device), and that have the potential to inform user
57 training.

58
59 Currently, quantifying the effectiveness of a given device, or the proficiency with which it is used,
60 remains limited by the available outcome measures [4]. Clinical tests often capture self-reported
61 capabilities (e.g. Orthotics and Prosthetics Users' Survey "OPUS" [5]), evaluate performance subjectively
62 (e.g. Assessment of capacity for myoelectric control [6]), or measure speed of performance of a pre-
63 defined set of tasks (e.g. Southampton Hand Assessment Procedure "SHAP" [7]). Research has
64 discussed the limitations with many of these measures, such as reliance upon self-report and/or
65 observer ratings [8-10]; self-report does not directly measure the person's physical capabilities and can
66 be influenced by subject bias, and observer-dependent measures are susceptible to (inter-/intra-) rater
67 bias, which inherently reduces reliability compared to performance-based measures in which the
68 administrator does not form part of the instrument. Previous research has also shown that whilst
69 important [10], speed of task completion is only one of several factors which characterize skilled

70 prosthetic use; other measures, notably gaze and kinematics may further enhance our understanding of
71 user performance and skill level [11].

72

73 Accordingly, Major et al. recently compared the kinematics of myoelectric prosthesis users and able-
74 bodied controls without known pathology [12]. Specifically, considering that motor variability (motor
75 variance across task repetition) has shown to decrease with skill acquisition [13, 14], and given the
76 redundant degrees of freedom (DoFs) in the upper body musculoskeletal architecture that permit
77 various task-equivalent motor strategies, Major et al. [12] focused on studying kinematic variability of
78 these DoFs. Their results showed that joint kinematic variability is higher in prosthesis users than
79 controls, and was correlated with years of experience of prosthesis use. Their findings suggest that
80 increased compensation may be reflected in increased joint kinematic variability above able-bodied
81 individuals.

82

83 In common with almost all studies of upper limb functional task performance, in [12] joint angle
84 trajectories were calculated as follows. Angle trajectories were first linearly normalized with respect to
85 time, and joint level kinematic variability was defined as the variability around a kinematic profile
86 averaged across multiple time-normalized trials. The standard deviation and coefficient of multiple
87 determination then served as outcome measures to characterize variability and repeatability,
88 respectively. However, non-cyclic kinematics are subject to two different aspects of trajectory
89 variability: temporal and amplitude variability (Figure 1). Specifically, the relative duration of different
90 phases of a given functional movement can vary from trial to trial, and linear time normalization of the
91 entire task cannot take this into account [15]. Hence, while these traditional measures can inform on
92 overall differences in movement variability, they remain limited in that they do not consider temporal
93 variability separately to variations in signal amplitude, yet this has shown to be advantageous in the
94 assessment of non-cyclic functional upper limb tasks [15,16].

95 Thies et al. previously introduced a novel methodology based on dynamic time warping (DTW) for curve
96 registration across multiple trials to calculate measures of amplitude and timing variability over entire
97 trajectories of functional movements [15]. In their approach a chosen target signal is warped to a
98 declared reference signal by compressing or stretching the target signal along the time-axis with respect
99 to the reference signal in a non-uniform manner. Warp Cost reflects the amount of time-warping
100 needed to achieve the best possible temporal match between curves and serves as a measure of
101 temporal variability. Following the time warping of signals, RMS error then informs on amplitude
102 variability. Separating out temporal from amplitude variability is of particular advantage during
103 processing of non-cyclic upper limb kinematics: we take the stand that DTW is a more appropriate
104 method to analyse kinematic inter-trial variability of the upper limbs during functional task performance
105 since it minimizes the mismatch of the different movement components (Figure 2).

106

107 A first demonstration of the DTW method involved characterization of acceleration trajectories derived
108 from an arm-worn accelerometer during performance of two daily-living activities in subjects with
109 stroke and matched controls. Findings showed increased timing variability for the stroke subjects as
110 compared to controls, and this outcome was reliably reproduced on a second test day one month later
111 [15]. This finding of increased variability following stroke was consistent with numerous previous
112 studies, which have generally used simpler tasks and discrete, rather than continuous, measures of
113 variability (e.g. variability of end point error in pointing tasks [17, 18]). A more recent study used the
114 DTW method to demonstrate differences in trajectory variability when comparing stroke survivors with
115 right and left hemisphere lesions, as well as to healthy controls [16]. They showed increased timing
116 variability in the paretic arm of stroke survivors with right compared with left hemisphere lesions and
117 further confirmed previous finding [15] of increased variability following stroke compared with controls.
118 The DTW method which assesses contributions of temporal and amplitude variability separately proved
119 particularly suitable to identify differences between left and right hemispheric stroke survivors.

120 Although already demonstrated for assessment of upper limb kinematics in people with stroke, the
121 potential and validity of this methodology to characterize upper limb movements in relation to
122 functional performance for upper limb prosthesis users has yet to be explored. Hence this paper
123 reports on the characterization of functional task performance with an upper limb myoelectric
124 prosthesis using the DTW method. The purpose of this retrospective study was to investigate whether
125 DTW is a valid tool for assessing temporal and amplitude variability of upper limb prosthesis kinematics
126 through a known-groups assessment (Study 1) and a responsiveness assessment (Study 2).

127

128 **2. METHODS**

129 In Study 1 we investigated the use of DTW to characterize upper limb function of myoelectric prosthesis
130 users and anatomically intact (AI) controls and its ability to discriminate between these two groups,
131 based on temporal and amplitude variability. In Study 2 we report on the changes in temporal and
132 amplitude variability with practice in using a myoelectric prosthesis simulator (AI subjects), to assess if
133 DTW can identify changes in temporal and amplitude variability resulting from practice of goal-oriented
134 tasks. Since accelerometers are wearable, inexpensive and clinically-accessible devices, we here apply
135 DTW to simulated accelerometer trajectories derived from position data, however, the method is
136 applicable to a range of kinematic data, including joint angle trajectories and data from other segment-
137 mounted inertial measurement units.

138

139 ***2.1 DTW for assessment of temporal and amplitude variability***

140 As previously described [15], the DTW method employed in these two studies utilized dynamic
141 programming [19] to separately quantify timing and amplitude variability across multiple trials. Using
142 custom software in Matlab (Mathworks, Natick, MA), the algorithm first time-warps a chosen target
143 signal to a declared reference signal by compressing or stretching the target signal along the time-axis
144 with respect to the reference signal in a non-uniform manner. Warp Cost is returned as a unitless

145 measure indicating the amount of time-warping needed to achieve the best possible temporal match
146 between curves. Warp Cost is hence reported as a measure of temporal variability between trials. Figure
147 3 stresses the need for DTW for accurate assessment of upper limb kinematic variability in an
148 anatomically intact subject, an anatomically intact subject using a prosthesis simulator, and an actual
149 prosthesis user. After time warping, the algorithm calculates the remaining root mean square error
150 (RMS Error) between signals after time-warping is complete. We interpret the reported RMS Error as a
151 measure of signal amplitude variations after temporal variations have been addressed.

153 **2.2 Study 1 (Known-groups assessment)**

154 Study 1 was carried out at Northwestern University, USA. Full details of the protocol are provided in [12].
155 Following ethical approval by the Northwestern University Institutional Review Board, six AI individuals (3
156 male, 35 ± 11 years of age) and seven myoelectric transradial prosthesis users (5 male, 49 ± 18 years of age,
157 20 ± 18 years of prosthesis experience) were recruited and tested. Subjects visited the lab on one occasion
158 and, after providing informed consent, performed five trials of three seated, goal-oriented tasks (selected
159 from the SHAP [7]): 1) lifting a carton and emptying liquid contents into a jar using their non-dominant or
160 prosthetic limb, 2) lifting and transferring a weighted container across a low-level barrier using their non-
161 dominant or prosthetic limb, and 3) lifting and transferring a tray across a low-level barrier using both
162 hands. The non-dominant limb of able-bodied individuals was chosen for sensible comparison with
163 prosthesis users whose prosthetic limb we assumed to act as the non-dominant limb [20]. The number of
164 trials (5) was comparable with other studies concerned with assessment of prosthesis kinematics [21, 22].
165 Subjects were asked to perform the task as quickly as possible and the start and end of each trial was
166 denoted by a button-push. Both groups also completed the entire SHAP protocol with their non-dominant
167 hand to assess general upper limb functional abilities. SHAP has shown to have good reliability and validity
168 for assessment of hand function [7], with scores of less than 100 indicating how impaired hand function
169 is. During each task, marker position approximating location of the radial and ulnar styloid processes were

170 collected and used to track the virtual wrist joint centre. Three markers on the forearm (radial styloid,
171 ulnar styloid, and medial epicondyle) were used to define the forearm local reference frame. The 3D
172 position data were collected at 120 Hz using a twelve camera motion capture system (Motion Analysis
173 Corporation, Santa Rosa, CA, USA). Wrist joint three-axis accelerations were calculated in the global
174 frame, then gravity was added to the vertical acceleration component. Finally, the acceleration vector
175 was rotated from the global to the forearm frame [23]. These simulated accelerometer data were used to
176 calculate inter-trial temporal (Warp Cost) and amplitude (RMS Error) variability [15].

177
178 This known-groups assessment was deemed to support validity of the methodology if the trends in the
179 variability assessed with DTW reflected those previously observed in joint-level kinematics [12], i.e., we
180 hypothesized that prosthesis users would demonstrate greater variability than controls. Moreover, use of
181 DTW in this study would identify individual contributions of temporal- and amplitude-specific variability
182 to overall movement variability. Data were statistically analysed using independent group t-tests to
183 compare mean differences in Warp Cost, RMS Error, and SHAP score between AI and prosthesis user
184 cohorts, and significance was evaluated based on equality of variances as estimated by the Levene's Test.

186 **2.3 Study 2 (Responsiveness assessment)**

187 Study 2 was carried out at the University of Salford, UK. Following ethical approval by the University of
188 Salford Research Ethics Committee, seven AI individuals (4 male, 6 right handed, 36 ± 10 years of age)
189 provided informed consent and were recruited to the study. AI subjects rather than novel myoelectric
190 prosthesis users were recruited because of the very small numbers of traumatic upper limb amputees
191 referred to limb fitting centres. For example, in 2004/5, there were just 54 new referrals of trans-radial
192 amputees in the UK. Subjects visited the lab on 9 occasions over approximately a 2-week period; full
193 details of the full protocol are published in [24], however, only a subset of visits is reported on here. On
194 their first visit, subjects were asked to perform a seated task which involved reaching with their

195 anatomic hand for a juice carton, picking it up and pouring the liquid into a cup, before returning it to its
196 original location, then moving their hand back to the original resting point (anatomic hand baseline). The
197 location of the carton, cup and starting point for the hand were fixed for each subject across all trials.
198 Subjects repeated the task 12 times. During their second functional task assessment as well as during
199 their final functional task assessment, subjects performed the same task with the same number of
200 repeats but with a custom-made myoelectric prosthesis simulator [24]. In between these prosthesis
201 simulator sessions, subjects carried out the SHAP on four occasions for practicing with the prosthesis
202 simulator. During task performance, 3D position data of a cluster of 4 reflective markers located on the
203 forearm were collected at 100 Hz using a ten camera Vicon 612[®] motion capture system (Vicon Motion
204 Systems, Los Angeles, USA). The position data of their anatomic hand baseline, their first prosthesis
205 simulator session, and their final session with the prosthesis simulator (after SHAP training) were then
206 used to calculate the simulated output of a three-axis accelerometer [23]. Subsequently, temporal and
207 trajectory variability within session were calculated. It was hypothesized that introduction of the
208 prosthesis would increase variability (anatomic baseline versus initial Prosthesis simulator session), and
209 that training through practice to use a prosthesis simulator would reduce variability. Following checks
210 for their normal distribution, warp cost and remaining RMS error were statistically analyzed using a one-
211 way repeated measures ANOVA (SPSS General Linear Model tab) with post-hoc Bonferroni correction
212 for Type 1 Error.

213

214 For all statistical analyses, the critical α was set at 0.05 to guide interpretation of the results, and
215 statistics were conducted using SPSS software (IBM, Armonk, New York).

216

217

218

219

3. RESULTS

3.1 Study 1 (Known-groups assessment)

Significant differences in temporal variability (Warp Cost) were found between prosthesis-users and able-bodied controls. Specifically, prosthesis users exhibited greater temporal variability than controls, and this was so for all three tasks (Figure 4 and Table 1). Results suggested that amplitude variability was greater for prosthesis users than able-bodied across tasks, but these group differences were not statistically significant ($P>0.05$ for all tasks, Figure 4 and Table 1). Average SHAP Index of Function scores for able-bodied and prosthesis users were $96(\pm 3 \text{ SD})$ and $53(\pm 12 \text{ SD})$ ($p<0.001$), respectively, suggesting lower upper limb functional abilities for prosthesis users.

3.2 Study 2 (Responsiveness assessment)

Clear changes in temporal variability emerged throughout the study period (Figure 5 (left) and Table 2). Specifically, when AI subjects were asked to use the prosthesis simulator for the first time, their temporal variability increased as compared to their baseline performance with the anatomical hand ($P=0.022$), but as they learned how to use the prosthesis simulator, their variability decreased again ($P=0.043$) and returned to levels similar to baseline ($P=0.267$). Changes in amplitude variability likewise emerged, although with a direction of continuous reduction in RMS Error throughout the study period (Figure 5 (right) and Table 2). Specifically, RMS Error slightly decreased from baseline as subjects were introduced to the prosthesis simulator ($P=1.000$), and a further reduction in RMS Error occurred with practice to use the simulator ($P=0.003$), interestingly to levels much lower than baseline ($P=0.043$).

4. DISCUSSION

The combined results from Studies 1 and 2 support the validity and usefulness of the DTW method for characterizing movement quality of task execution when using an upper limb prosthesis. Study 1 found significant differences in temporal inter-trial variability between prosthesis users and controls, but not in amplitude variability. This finding demonstrates for the first time the nature of differences in trial-to-trial variability between experienced users of myoelectric prostheses and controls. Specifically, by separating out the two elements of trajectory variability, DTW revealed the primary contribution of temporal variability to overall movement quality, with less apparent contributions of amplitude variability. Moreover, that prosthesis users exhibited greater kinematic variability as compared to controls across all three tasks along with reduced function, as quantified by lower SHAP scores, is in agreement with previous findings [12], thereby supporting the validity of this method. It should be noted that one of the possible reasons for the lack of statistical significance in amplitude variability was the low statistical power due to a small sample size. Although consistent group differences in amplitude variability existed across tasks, with magnitudes greater than those found with training in Study 2, these differences were not large enough to reach significance given the within-group variability.

Although not unexpected, no-one has previously demonstrated that variability reduces with practice with a prosthesis simulator. In Study 2 we investigated the extent by which temporal and amplitude variability each contribute to this outcome and demonstrated that temporal variability in a carton pouring task increased considerably on first use of a prosthesis simulator, then declined with goal-oriented training (SHAP). Temporal variability hence showed to be responsive to effects of training. Consistent with the findings in Study 1, amplitude variability showed less clear changes, especially on first introduction of the prosthesis simulator. Two limitations of Study 2 are that AI subjects used a prosthesis simulator and performed only one functional task. Therefore further research involving actual

269 myoelectric prosthesis users and a more comprehensive task protocol is required to substantiate the
270 findings of Study 2.

271

272 Consistent with our previous study in stroke [15] temporal variability, as compared to amplitude
273 variability, emerged as the more insightful measure. As all of the tasks studied involved acquiring and
274 releasing objects using the prosthetic hand, and since opening the hand to acquire or release an object
275 is a common challenge in prosthesis control, then hesitations upon grasp and release may be one of the
276 sources of the higher timing variability seen in prosthesis users. It is noteworthy that temporal variability
277 varied significantly across tasks (see Table 1), each of which involved a single grasp and release, and
278 further work is needed to interpret this finding. Furthermore, given the trends observed in Studies 1 and
279 2, higher prosthesis user amplitude variability and a decrease with simulator training respectively, the
280 contribution of amplitude variability to movement quality should be explored further. Previous work has
281 suggested that below-elbow amputees are able to generate an accurate internal model of the prosthetic
282 limb [25] which implies self-integration of the limb to refine relationships between physiological input
283 and performance output. For example, one explanation for the decrease in amplitude variability with
284 practice (Figure 5) is that learning to use a prosthesis simulator with reduced DoFs may require some
285 development of a new internal model with training to minimize limb amplitude variability. The increase
286 (Prosthesis 1, Figure 5) and subsequent decrease (Prosthesis Final, Figure 5) in temporal variability upon
287 introduction to the prosthesis simulator would be reflective of skill acquisition.

288

289 Overall, analysing forearm accelerations using the DTW method appears to be a valid method for
290 quantifying movement quality of upper limb prosthesis use during the execution of goal-oriented tasks.
291 The information delivered from such assessment offers a valuable, objective outcome for monitoring
292 rehabilitation progress that would complement other performance-based and self-report clinical
293 outcome measures. A rich set of outcome data would aid in development of more appropriate, patient-

294 centric training programs with the aim of maximizing functional performance and minimizing potential
295 for device abandonment. Yet, further work is needed to understand the implications of our work for
296 clinical training. We have shown that in simulator users both amplitude and temporal trajectory
297 variability decrease with practice, suggesting our metrics may be of value in assessing skill. However,
298 research is needed to understand whether patients would benefit from training specifically targeted at
299 reducing variability.

300

301 Importantly, the studies reported here used camera based techniques to derive overall task completion
302 time and simulated accelerometer trajectories. However, both of these parameters could be derived
303 from a forearm-mounted accelerometer and hence the approach offers the potential for clinicians to
304 characterise both overall task completion time and trial-trial temporal and trajectory variability using
305 low cost instrumentation. Accelerometers have previously been used for classification of hand
306 movements [26, 27], and this study shows their potential in assessment of kinematic variability as an
307 aspect of movement quality. Future work should continue to explore use of wearable devices as a
308 simple, reliable, and clinically-accessible method for assessing prosthesis-use skill. When combined with
309 the use of low cost instrumentation, reliability of the DTW method for assessing prosthesis user
310 movement quality should be investigated to complete an evaluation of its psychometric properties.

311

312 **ACKNOWLEDGEMENTS**

313 This research was supported in part by a Career Development Award (Award #1K2RX001322-01A1)
314 from the United States (U.S.) Department of Veterans Affairs Rehabilitation Research and Development
315 Service,, the David Rubin, MD, Enrichment Fund, and the Department of Education National Institute on
316 Disability and Rehabilitation Research (Grant No. H133E080009).

317

318

319 **DECLARATIONS**

320 **Ethics approval and consent to participate:** For testing of human subjects, Study 1 (Known-groups
321 assessment) received ethical approval from the Northwestern University Institutional Review Board,
322 USA (Ref # STU00028580), whilst Study 2 (Responsiveness Assessment) received ethical approval from
323 the University of Salford Research Ethics Committee (Ref # REPN09/174). All participants provided
324 informed consent. Animals were not part of the study.

325 **Conflicts of interest:** The authors declare that no financial and personal relationships with other people
326 or organizations exist that could have inappropriately influenced (biased) this work.

327

328 **AUTHOR'S CONTRIBUTIONS**

329 All substantial contributions of authors to the paper were as follows: (1) the conception and design of
330 the study (all), or acquisition of data (MS, RS), or analysis and interpretation of data (SBT, LPJK, MJM);
331 (2) drafting the article or revising it critically for important intellectual content (all); (3) final approval of
332 the version to be submitted (all).

333

334 **REFERENCES**

335 [1] Fougner A, Stavadahl O, Kyberd PJ, Losier YG, Parker PA. Control of upper limb prostheses: terminology
336 and proportional myoelectric control-a review. IEEE Trans Neural Syst Rehabil Eng 2012; 20: 663-77.

337 [2] McFarland LV, Hubbard Winkler SL, Heinemann AW, Jones M, Esquenazi A. Unilateral upper-limb loss:
338 satisfaction and prosthetic-device use in veterans and servicemembers from Vietnam and OIF/OEF
339 conflicts. J Rehabil Res Dev 2010; 47: 299-316.

340 [3] Ostlie K, Lesjø IM, Franklin RJ, Garfelt B, Skjeldal OH, Magnus P. Prosthesis rejection in acquired major
341 upper-limb amputees: a population-based survey. Disabil Rehabil Assist Technol 2012; 7: 294-303.

- 342 [4] Resnik L, Borgia M, Silver B, Cancio J. Systematic Review of Measures of Impairment and Activity
343 Limitation for Person with Upper Limb Trauma and Amputation. Arch Phys Med Rehabil 2017. [Epub
344 ahead of print]
- 345 [5] Heinemann AW, Bode RK, O'Reilly C. Development and measurement properties of the orthotics and
346 prosthetics users' survey (OPUS): a comprehensive set of clinical outcome instruments. Prosthet Orthot
347 Int 2003; 27: 191–206.
- 348 [6] Hermansson LM, Bodin L, Eliasson AC. Intra- and inter-rater reliability of the assessment of capacity
349 for myoelectric control. J Rehabil Med 2006; 38: 118 –23.
- 350 [7] Light CM, Chappell PH, Kyberd PJ. Establishing a standardized clinical assessment tool of pathologic
351 and prosthetic hand function: normative data, reliability, and validity. Arch Phys Med Rehabil 2002; 83:
352 776-83.
- 353 [8] Krakauer JW. Arm function after stroke: from physiology to recovery. Semin Neurol 2005; 25: 384-95.
- 354 [9] Hummel FC, Celnik P, Pascual-Leone A, Fregni F, Byblow WD, Buetefisch CM, Rothwell J, Cohen LG,
355 Gerloff C. Controversy: Noninvasive and invasive cortical stimulation show efficacy in treating stroke
356 patients. Brain Stimul 2008; 1: 370-82.
- 357 [10] Bouwsema H, Kyberd PJ, Hill W, van der Sluis CK, Bongers RM. Determining skill level in myoelectric
358 prosthesis use with multiple outcome measures. J Rehabil Res Dev 2012; 49: 1331-48.
- 359 [11] Bongers RM, Kyberd P, Bouwsema H, Kenney L, Plettenburg DH, Van der Sluis CK. Bernstein's levels
360 of construction of movements applied to upper limb prosthetics. J Pros Orth 2012; 24: 67–76.
- 361 [12] Major MJ, Stine RL, Heckathorne CW, Fatone S, Gard SA. Comparison of range-of-motion and
362 variability in upper body movements between transradial prosthesis users and able-bodied controls
363 when executing goal-oriented tasks. J Neuroeng Rehabil 2014; 11:132

- 364 [13] Stergiou N, Harbourne R, Cavanaugh J. Optimal movement variability: a new theoretical perspective
365 for neurologic physical therapy. *J Neurol Phys Ther* 2006; 30: 120-9
- 366 [14] Shmuelof L, Krakauer JW, Mazzoni P. How is a motor skill learned? Change and invariance at the
367 levels of task success and trajectory control. *J Neurophysiol* 2012; 108: 578-94.
- 368 [15] Thies SB, Tresadern PA, Kenney LP, Smith J, Howard D, Goulermas JY, et al. Movement variability in
369 stroke patients and controls performing two upper limb functional tasks: a new assessment
370 methodology. *J Neuroeng Rehabil* 2009; 6:2.
- 371 [16] Freitas SM, Gera G, Scholz JP. Timing variability of reach trajectories in left versus right hemisphere
372 stroke. *Brain Res* 2011; 1419: 19-33
- 373 [17] Cirstea MC & Levin MF. Compensatory strategies for reaching in stroke. *Brain* 2000; 123: 940-53.
- 374 [18] Gordon J, Ghilardi MF, Ghez C. Accuracy of planar reaching movements. I. Independence of
375 direction and extent variability. *Exp Brain Res* 1994; 99: 97-111
- 376 [19] Cormen TH, Leiserson CE, Rivest RL, Stein C (2001) Introduction to algorithms. 2. Boston: MIT Press.
- 377 [20] Philip BA, Frey SH. Compensatory changes accompanying chronic forced use of the nondominant
378 hand by unilateral amputees. *J Neurosci* 2014; 34: 3622-31.
- 379 [21] Bertels T, Schmalz T, Ludwigs E. Objectifying the functional advantages of prosthetic wrist flexion. *J*
380 *Prosthet Orthot* 2009; 21: 74-78.
- 381 [22] Carey SL, Jason Highsmith M, Maitland ME, Dubey RV. Compensatory movements of transradial
382 prosthesis users during common tasks. *Clin Biomech* 2008; 23: 1128-35.
- 383 [23] Thies SB, Tresadern P, Kenney L, Howard D, Goulermas JY, Smith C, Rigby J. Comparison of linear
384 accelerations from three measurement systems during "reach & grasp". *Med Eng Phys* 2007; 29: 967-72.

- 385 [24] Sobuh MM, Kenney LP, Galpin AJ, Thies SB, McLaughlin J, Kulkarni J, et al. Visuomotor behaviours
386 when using a myoelectric prosthesis. *J Neuroeng Rehabil* 2014; 11:72.
- 387 [25] Schabowsky CN, Dromerick AW, Holley RJ, Monroe B, Lum PS. Trans-radial upper extremity
388 amputees are capable of adapting to a novel dynamic environment. *Exp Brain Res* 2008; 188: 589-601.
- 389 [26] Soma H, Horiuchi Y, Gonzalez J, Yu W. Preliminary results of online classification of upper limb
390 motions from around-shoulder muscle activities. *IEEE Int Conf Rehabil Robot*. 2011.
- 391 [27] Atzori M, Gijssberts A, Müller H, Caputo B. Classification of hand movements in amputated subjects
392 by sEMG and accelerometers. *Conf Proc IEEE Eng Med Biol Soc* 2014; 2014: 3545-9.

393

394 TABLES

395 Table 1. Known-groups assessment (Study 1)

	Group	Carton Pouring		Weighted Container Transfer		Tray Transfer	
		Mean (SD)	<i>P</i> [95% CI]	Mean (SD)	<i>P</i> [95% CI]	Mean (SD)	<i>P</i> [95% CI]
Warp Cost	Anatomically Intact	85.80 (27.14)	0.02 [-158.55, -18.33]	6.92 (2.31)	0.004 [-100.63, -29.03]	13.55 (9.14)	0.019 [-73.96, -9.40]
	Prosthesis User	174.24 (74.48)		71.75 (38.71)		55.23 (34.70)	
RMS Error [m/s²]	Anatomically Intact	0.60 (0.09)	0.07 [-934.53, 43.69]	0.93 (0.28)	0.127 [-750.20, 106.65]	1.26 (0.41)	0.164 [-833.74, 160.12]
	Prosthesis User	1.04 (0.53)		1.25 (0.40)		1.60 (0.41)	

396

397 Group mean (standard deviation “SD”) and statistical t-test results for Warp Cost and RMS Error for the
 398 three functional tasks. 95%CI: 95% Confidence Interval of Mean Difference.

399

400 Table 2. Responsiveness assessment (Study 2)

	Warp Cost		RMS Error [m/s ²]	
	Mean (SD)	<i>P</i> [†] [95% CI]	Mean (SD)	<i>P</i> [†] [95% CI]
Anatomic	60.45 (17.02)	0.022 [-141.55; -13.07]	0.47 (0.09)	1.000 [-0.15; 0.19]
Prosthesis 1	137.77 (43.92)		0.45 (0.07)	
Prosthesis 1	137.77 (43.92)	0.043 [2.15; 125.48]	0.45 (0.07)	0.003 [0.05; 0.18]
Prosthesis Final	73.95 (19.27)		0.33 (0.04)	
Prosthesis Final	73.95 (19.27)	0.267 [-8.38; 35.37]	0.33 (0.04)	0.043 [-0.26; -0.01]
Anatomic	60.45 (17.02)		0.47 (0.09)	

401 †Adjustment for multiple comparisons: Bonferroni.

402 Group mean (standard deviation “SD”) of Warp Cost and RMS Error for AI subjects at baseline (anatomic
 403 hand) and during learning to use a prosthesis simulator (myoelectric prosthesis) together with repeated
 404 measures GLM pairwise comparisons for test sessions. 95%CI: 95% Confidence Interval of Mean
 405 Difference.

406 **FIGURE CAPTIONS**

407 **Figure 1. Illustration of temporal and amplitude variability.**


408 **Figure 2. Illustration of the effects of uniform time normalization as compared to DTW.** Example
409 (adapted from Thies et al. 2009): “drinking from a glass” involves a reach forward, grasp of the glass,
410 lifting, drinking and replacing the glass onto the table top. Note that for uniform time normalization
411 (left) trials remain inadequately aligned, as evident from the mismatch of the different movement
412 components, thereby leading to inappropriate estimation of inter-trial variation in signal amplitude
413 when RMS Error is calculated subsequently. This is not the case for DTW (right).

414 **Figure 3. Use of time-normalization versus non-linear time warping for assessment of upper limb**
415 **kinematic variability.** Example plots show distal-to-proximal forearm acceleration for an anatomically
416 intact individual (top), an anatomically intact individual using a prosthesis simulator (middle), and an
417 amputee (bottom), each pouring juice from a carton into a glass. Shown are original signals of 2 trials
418 (left), the same signals after time normalization (middle) and after time warping (right). A mismatch of
419 movement components remains after time normalization, whilst temporal alignment is optimized
420 through use of DTW for more accurate estimation of amplitude variability.

421 **Figure 4. Known-groups assessment (Study 1).** Group means and corresponding standard deviations for
422 temporal variability (Warp Cost, left) and amplitude variability (RMS Error, right) for all functional tasks.


423 **Figure 5. Responsiveness assessment (Study 2).** Group means and corresponding standard deviations
424 for temporal variability (Warp Cost, left) and amplitude variability (RMS Error, right). Anatomic: baseline
425 with anatomic hand; Prosthesis 1: first session with a myoelectric prosthesis simulator, Prosthesis Final:
426 final session with a prosthesis simulator (after four SHAP training sessions).

427

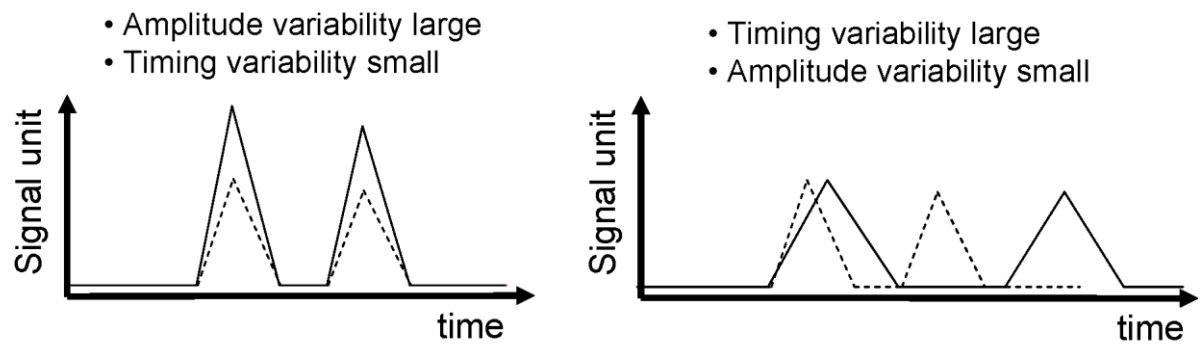


429 **Figure 1.**


"Drinking from a glass"

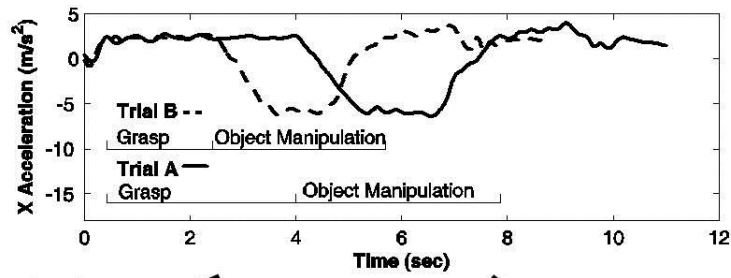

"% movement cycle" method

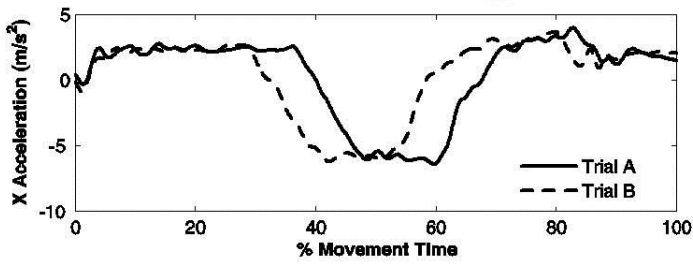

Dynamic Time Warping

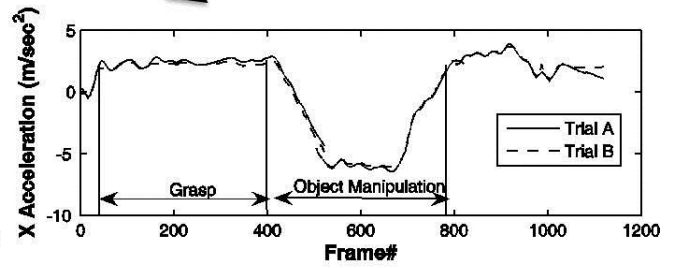

431


432 Figure 2.

433

434

435


Healthy subject anatomic arm “carton pouring task”:

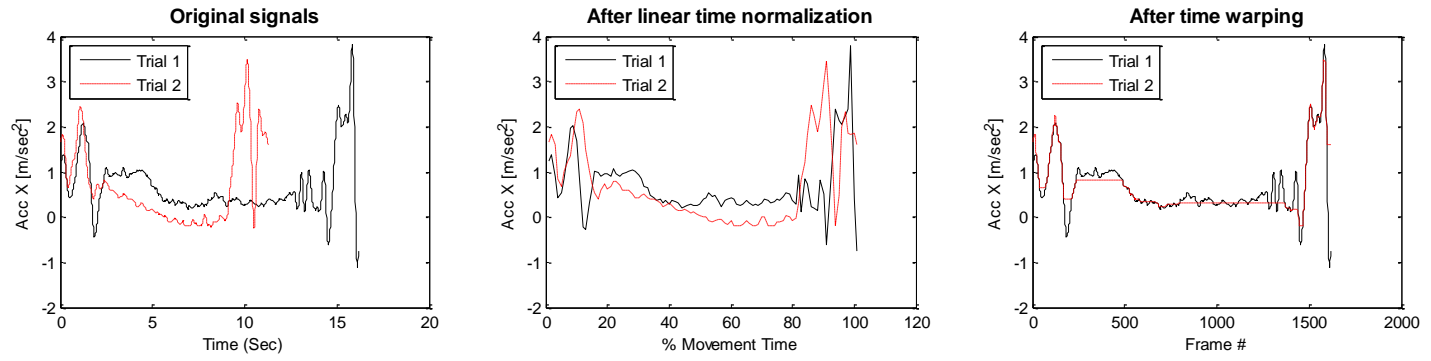

436

437

Healthy subject prosthesis simulator “carton pouring task”:

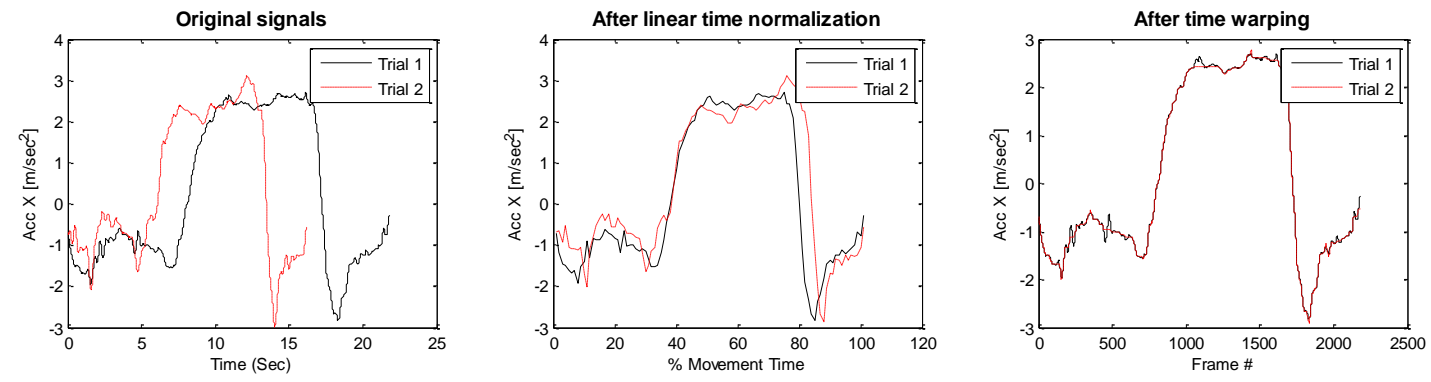

438

439

Myoelectric prosthesis user “carton pouring task”:


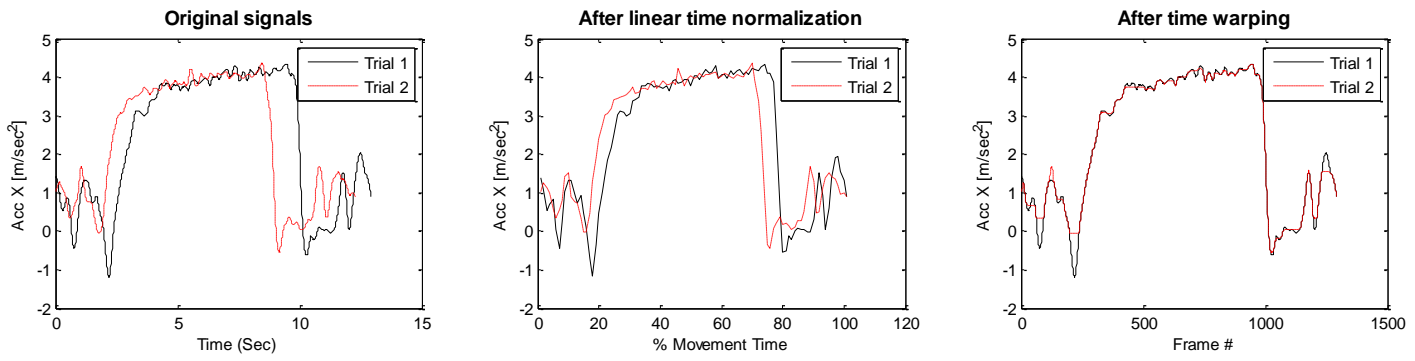


Figure 3.

441

442


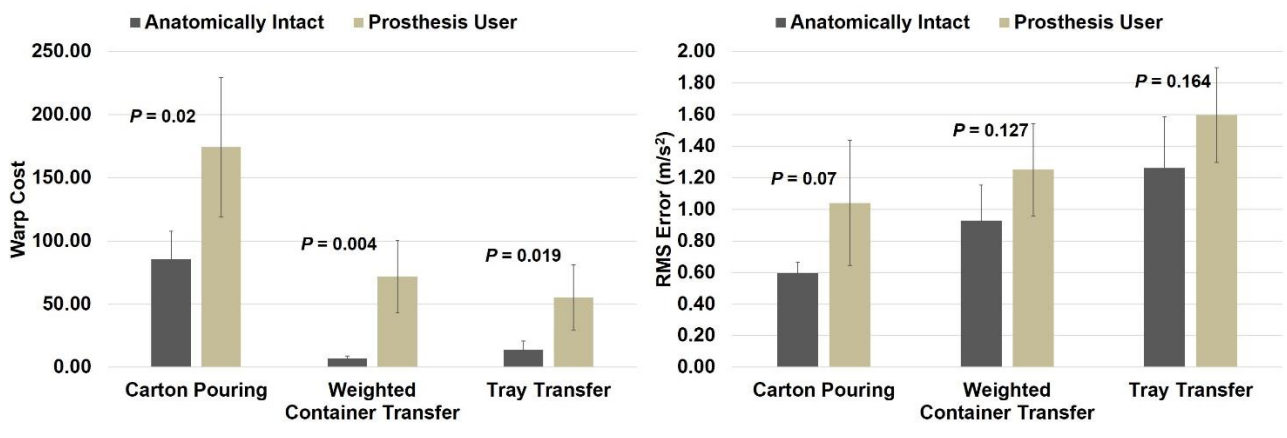


443

444 **Figure 4.**

445

446

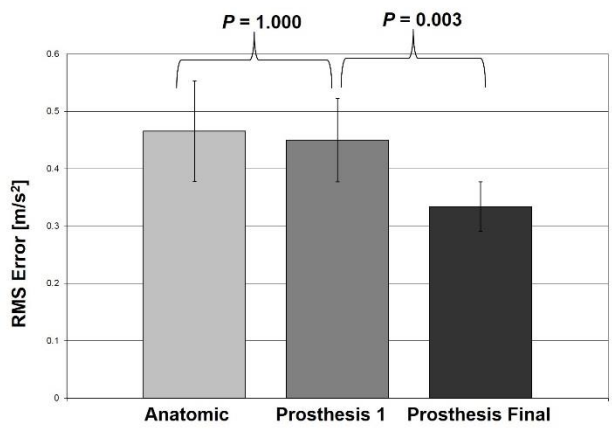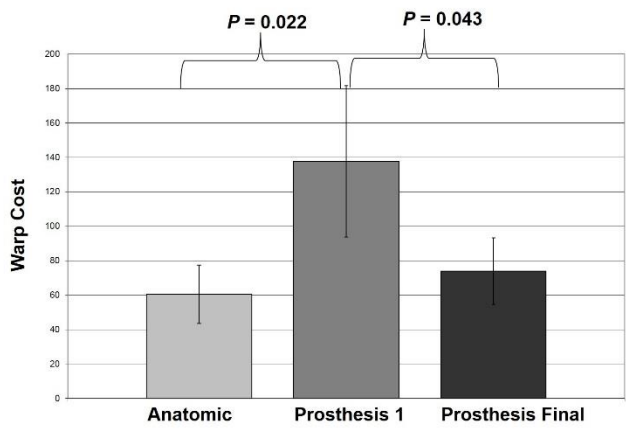

447

448 **Figure 5.**